

UT371/372 Operating Manual



Tachometer

Overview

This Operating Manual covers safety information related to the Tachometer. Please read the relevant information carefully and observe all the **Warnings** and **Notes** strictly.

Model UT371/UT372 is a stable, safe and reliable digital non-contact Tachometer. This Tachometer can measure RPM and counts. RPM range is 10 ~ 99999 while counts range is 0 ~ 99999.

Unpacking Inspection

Open the package case and take out the Meter. Check the following items carefully for any missing or damaged part:

| Item | Description | Qty |
|------|----------------------------------|-----------|
| 1 | English Operating Manual | 1 piece |
| 2 | Reflecting Tape | 10 pieces |
| 3 | USB Interface Cable (UT372 only) | 1 piece |
| 4 | Software (UT372 only) | 1 piece |
| 5 | 1.5V Battery (LR6) | 4 pieces |

In the event you find any missing or damaged item, please contact your dealer immediately.

Safety Information

This Meter complies with IEC61010-031 and IEC61326 standards as well as Pollution Degree 2 requirement

Use the Meter only as specified in this operating manual, otherwise the protection provided by the Meter may be impaired.

In this manual, a **Warning** identifies conditions and actions that pose hazards to the user, or may damage the Meter or the equipment under test.

A **Note** identifies the information that user should pay attention to.

Warning

- Before using the Meter inspect the case. Do not use the Meter if it is damaged or the case (or part of the case) is removed. Look for cracks or missing plastic.
- Do not use or store the Meter in an environment of high temperature, humidity, explosive, inflammable and strong magnetic field. The performance of the Meter may deteriorate after dampened.

- Do not point laser directly at eye.
- Replace the battery as soon as the battery indicator appears. When the battery is between 4.5V ~ 4.8V, the battery indicator appears. When the battery is between 4.3V ~ 4.5V, battery indicator blinking, the Meter will be turned off after 1 minute.
- When opening the battery door, make sure the Meter is powered off.
- When servicing the Meter, use only the replacement parts with the same model or identical electrical specifications.
- The internal circuit of the Meter shall not be altered at will to avoid damage of the Meter and any accident.
- Soft cloth and mild detergent should be used to clean the surface of the Meter when servicing. No abrasive and solvent should be used to prevent the surface of the Meter from corrosion, damage and accident.
- Turn the Meter off when it is not in use and take out the battery when not using for a long time.
- Constantly check the battery as it may leak when it has been using for some time, replace the battery as soon as leaking appears. A leaking battery will damage the Meter.

International Electrical Symbols

| | |
|--|---|
| | Warning. Refer to the Operating Manual |
| | Low Battery Indication |
| | Conforms to Standards of European Union |

The Meter Structure (See Figure 1)

- ① Tachometer Light Source.
- ② LCD Display.
- ③ USB Port (UT372 only)
- ④ Housing
- ⑤ Functional Buttons

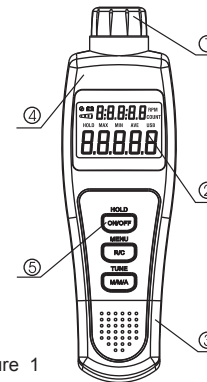


Figure 1

Functional Buttons

The table below offers information about the functional button operations.

| Button | Operation Performed |
|---------------|---|
| ON/OFF | <ul style="list-style-type: none"> ● Press once to turn the meter on. ● Press and hold for 1 second to turn it off. ● When measuring RPM and Counts, press once to enter the Hold mode. Press it again to exit hold mode. |
| R/C | <ul style="list-style-type: none"> ● When measuring RPM and Counts, press it to toggle between RPM and Counts feature. ● Press and hold for 1 minute to enter setup feature, the LCD displays USB. After that, each pressing steps through LED / SR / AOFF / CLK / settings, then exits the setup and accesses RPM or Count, You could press ON/OFF button to exit setup mode and return to normal measurement mode at any time. |
| M/M/A | <ul style="list-style-type: none"> ● Press this button to choose Max./Min./Average/Zeroing/Setting options. ● Under Tach measurement mode, press M/M/A button to select MAX/MIN/AVE and normal measurements. ● After entering USB/LED/SR/AOFF/CLK mode, press this button to set to 0/ 1 and adjust the time. |

Setup

A. USB

Press **R/C** button to select USB feature after turning on the Meter. Then press **M/M/A** button to set to 0 or 1. 0 represents disabling USB and 1 for enabling USB.

B. LED

Press **R/C** button to select LED feature after turning on the Meter. Then press **M/M/A** button to set to 0 or 1. 0 represents disabling LED laser and 1 for enabling the laser.

C. SR (Sampling Rate)

Press **R/C** button to select SR feature after turning on the Meter. Then press **M/M/A** button to adjust within 005 ~ 255. Press and hold **M/M/A** button to access quick setting.

D. AOFF

Press **R/C** button to select AOFF feature after turning on the Meter. Then press **M/M/A** button to set to 0 or 1. 0 represents disabling auto power off and 1 for enabling the function.

With the function enabled, the meter will automatically power off if buttons are inactive for 10minutes. Press ON/OFF again to wake up the meter.

E. CLK

Press **R/C** button to select CLK feature after turning on the Meter. Then press **M/M/A** button to set to 0 or 1. 0 is for h:m time format and 1 for m:s format.

Display Symbols (see figure 2)

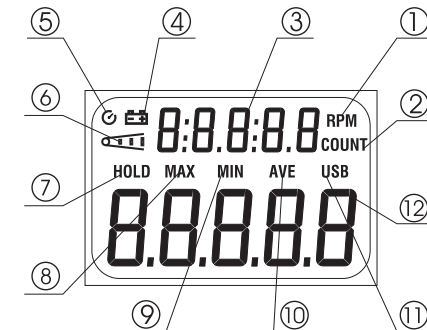


Figure 2

| Number | Meaning |
|--------|--------------------------------|
| 1 | Unit of Tachometer |
| 2 | Unit of Counts |
| 3 | Time |
| 4 | The battery is low. |
| 5 | Indicator of Sleep Mode |
| 6 | Measurement of RPM and Counts |
| 7 | Data Hold is on |
| 8 | Display of Maximum reading |
| 9 | Display of Minimum reading |
| 10 | Display of Average reading |
| 11 | USB is on |
| 12 | Display of Measurement reading |

Measurement Operation

Warning

- To reserve battery, the USB feature will be automatically off when the Meter is restarted. The other setting remains unchanged.
- The Time will be off after the HOLD feature is enabled. The time will be on again after existing HOLD mode.

A. RPM Measurement (See Figure 3)

Warning

- Do not point laser directly at eyes.
- To avoid the rotating object touching the meter and cause any injury or damage to the meter during the measurement, please keep the meter more than 50mm away from the tested target.

To carry out RPM measurement, follow the following procedure:

1. Attach a piece of reflecting tape to the object under test.
2. Position the meter firmly on desired location. Hold the meter and keep its light source 50~200mm away from the object under test.
3. Press **ON/OFF** button, the Meter is default to enter the RPM measurement mode. Point the Tachometer light source to reflective tape, The deviation from the ideal right-angle should not be greater than 30°.
4. The LCD displays the RPM reading.

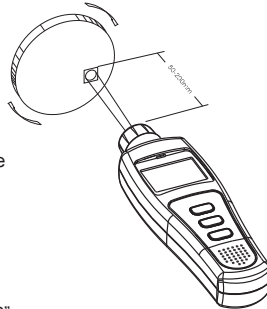


Figure 3

- Note:**
1. When measuring RPM, the LCD displays "0.0000" if there is no signal within 7 seconds.
 2. When the RPM is greater than 99999, the LCD displays OL.

B. Counts

Self-lighted Counts (See Figure 4)

1. Position the meter firmly on desired location. Hold the meter and keep its light source 50~200mm away from the targets.
2. Press the **ON/OFF** button
3. Press the **R/C** button to select Count mode.
4. Point the Tachometer light source to the objects under count. The deviation from the ideal right-angle should not be greater than 30°.
5. The LED scans the objects under count, counts the number and displays the total value.

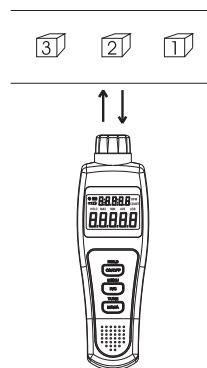


Figure 4

- Note:**
1. The object under count must be reflective, otherwise Counts feature cannot be used

Receiving Light Source Outside (See Figure 5)

1. Position the meter firmly on desired location. Hold the meter and keep its light source 50~200mm away from the targets. The deviation from the ideal right-angle pointing should not be greater than 30°.
2. Locate the Meter, objects under counts and light source as shown in Figure 5
3. Press **ON/OFF** button
4. Turn the LED off, refer to page 9 point B.
5. Then press **R/C** button to select Counts mode.
6. When the objects under count pass between the meter and light source, the meter count the number and display the total value.

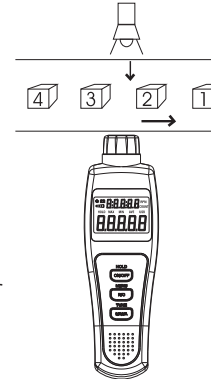


Figure 5

Note:

1. Under the count mode, when the total count the Meter displays OL and hold the data.
2. Press **M/M/A** button to zero the Counts.
3. Press **ON/OFF** to re-start Counting.

C. Data Transferring and USB (UT372 Only, See Figure 6)

Connect the meter to PC with use of USB cable. See Figure 6.

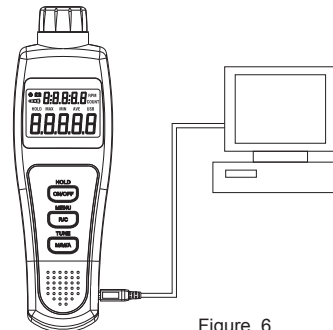


Figure 6

Specifications

A. General Specifications

- Display: 5 digits LCD display, Maximum display 99999.
- Overloading: Display **OL**.
- Low Battery Indication: Display
- Sampling Rate: Adjustable from 5ms~255ms.
- Sensor Type: Photo diode and laser tube
- Measurement Distance: 50mm ~ 200mm
- Drop Test: one meter
- Power: 4pcs x 1.5V batteries (AA)
- Dimensions: 184 x 56 x 34mm
- Weight: Approximate 100g (excluding battery)

B. Environmental Requirements

- For indoor use only.
- Altitude: 2000m
- Temperature and humidity:
 - * Operating:
 - 0°C~30°C(≤85%R.H)
 - 30°C~40°C (≤75%R.H)
 - 40°C~50°C (≤45%R.H)
 - * Storage:
 - 20°C~ +60°C(≤85%R.H)
- Safety/ Compliances: IEC61010-031, IEC61326, IEC 61010-1 pollution degree 2.
- Certification:

Accuracy Specifications

Accuracy: ±(a% reading + b digits), calibration per year.
 Operating temperature: 23°C±5°C
 Operating humidity: ≤80%RH
 Temperature Coefficient: 0.1 x (accuracy) / °C

A. RPM

| Range | Resolution | Accuracy |
|-------------------|-------------|------------|
| 10~99.999 r/min | 0.001 r/min | ±(0.04%+2) |
| 100~999.99 r/min | 0.01 r/min | |
| 1000~9999.9 r/min | 0.1 r/min | |
| 10000~99999 r/min | 1 r/min | |

B. Counts

| Range | Resolution | Max. Input Frequency |
|----------|------------|-----------------------|
| 0~ 99999 | 1 digit | 10kHz, Pulse Width 5% |

MAINTENANCE

This section provides basic maintenance information including battery replacement instruction.

Warning

Do not attempt to repair or service your Meter unless you are qualified to do so and have the relevant calibration, performance test, and service information.

Do not attempt to open the back housing to avoid damaging the Meter or affecting the accuracy.

A. General Service

- Periodically wipe the case with a damp cloth and mild detergent. Do not use abrasives or solvents.
- Turn the Meter power off when it is not in use.
- Take out the battery when it is not using for a long time.
- Do not use or store the Meter in a place of humidity, high temperature, explosive, inflammable and strong magnetic field.

B. Replacing the Battery (See Figure 7)

1. Press **ON/OFF** to turn the Meter off.
2. Turn the Meter's front case down.
3. Remove the screw from the battery door, and separate the battery door from the case bottom.
4. Take out the old batteries and replace with 4 x 1.5V battery (AA).
5. Rejoin the case bottom and the battery compartment, and reinstall the screw.




Figure 7

* END *

This operating manual is subject to change without notice.